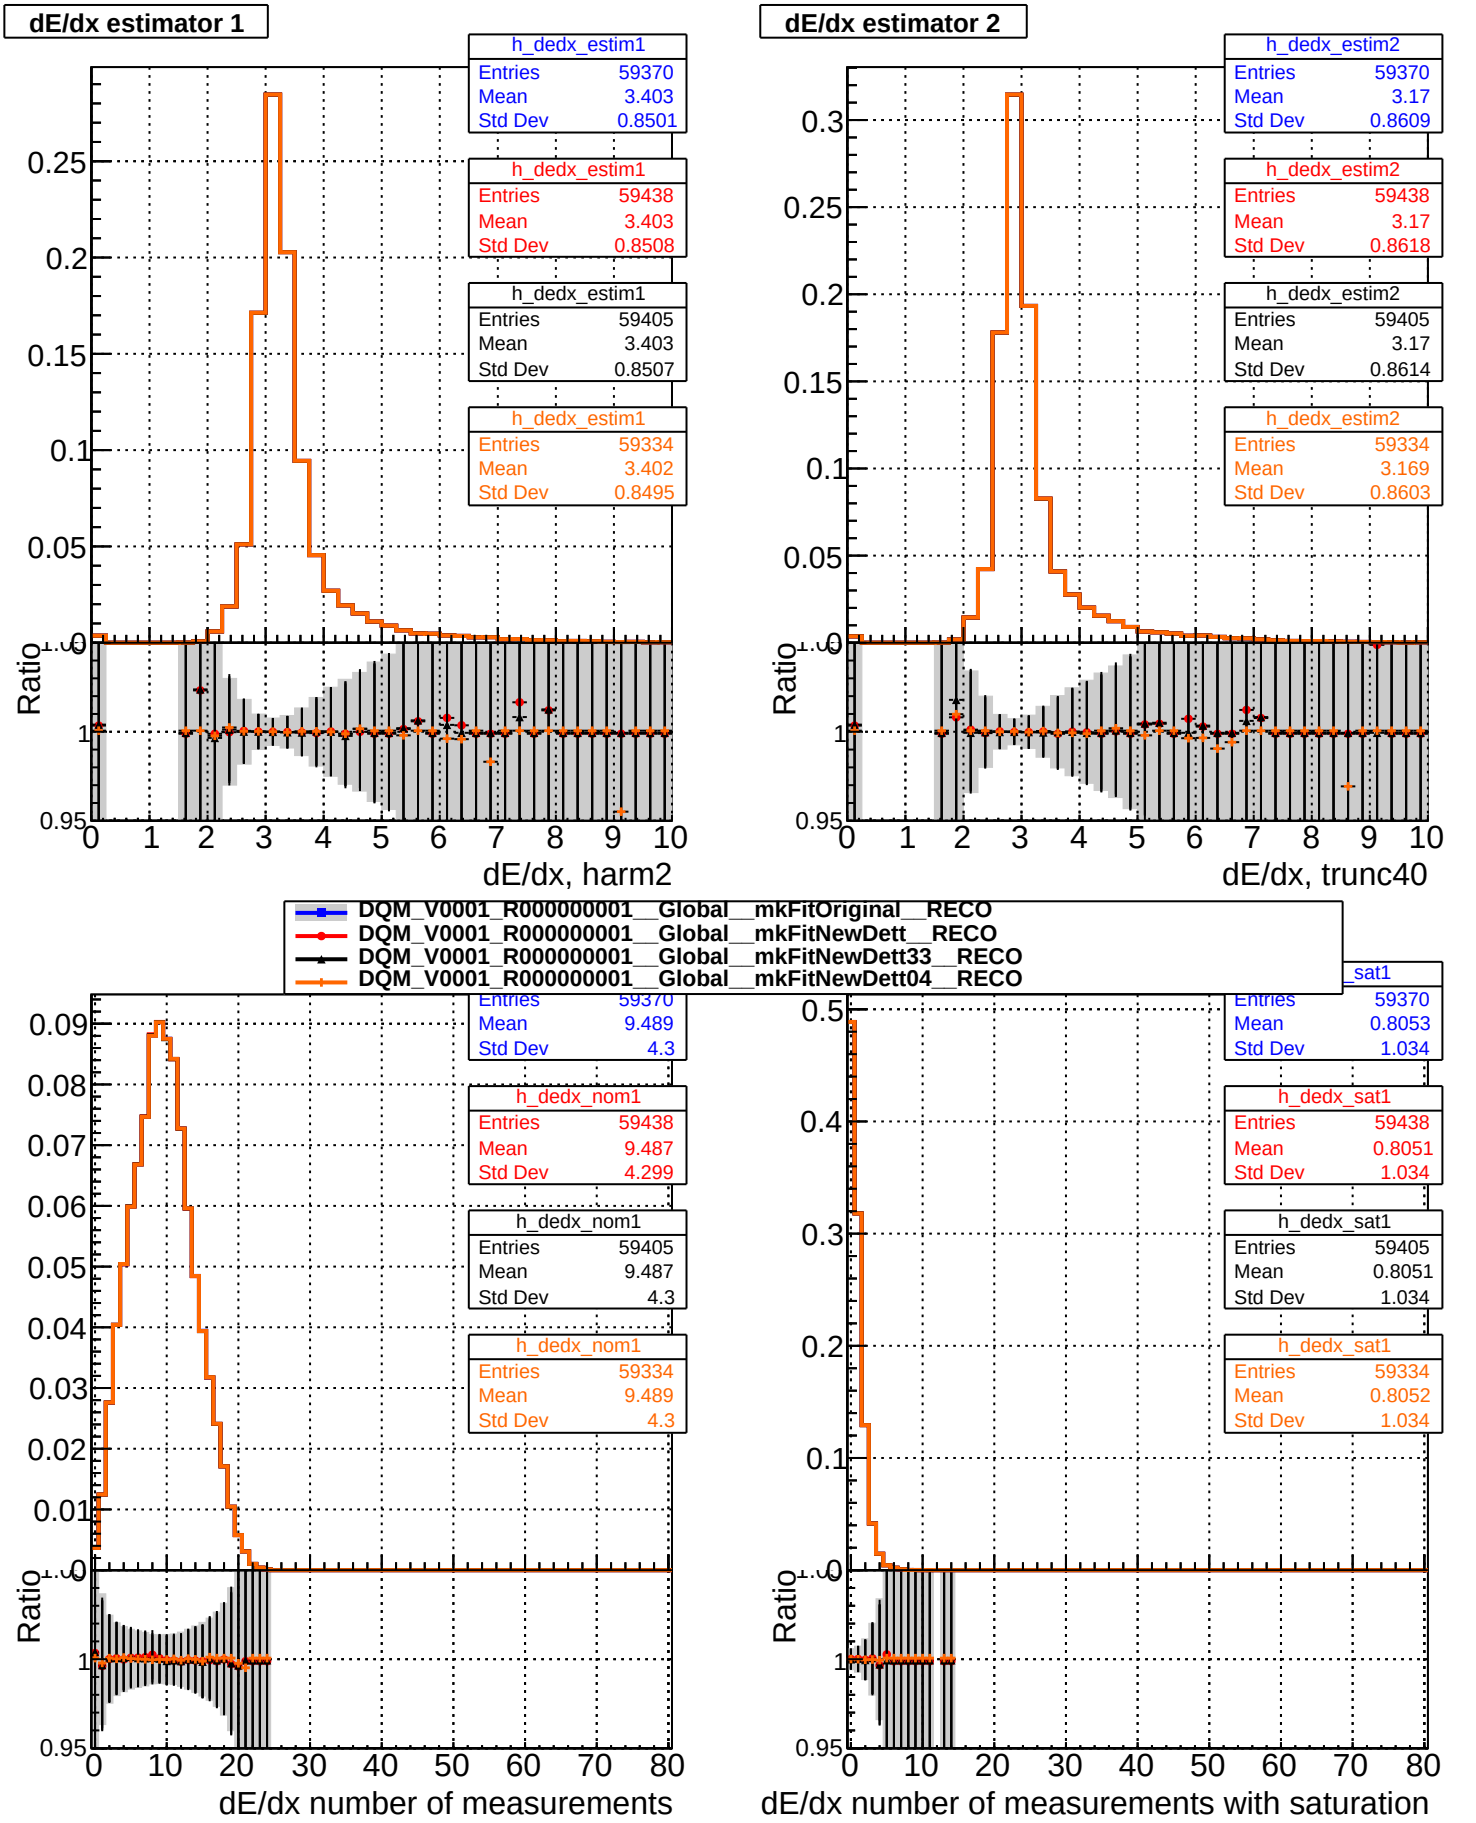
dE/dx estimator 1
h_dedx_estim1
Entries 59370
Mean 3.403
Std Dev 0.8501
h_dedx_estim1
Entries 59438
Mean 3.403
Std Dev 0.8508
h_dedx_estim1
Entries 59405
Mean 3.403
Std Dev 0.8507
h_dedx_estim1
Entries 59334
Mean 3.402
Std Dev 0.8495
Ratio
dE/dx, harm2
dE/dx estimator 2
h_dedx_estim2
Entries 59370
Mean 3.17
Std Dev 0.8609
h_dedx_estim2
Entries 59438
Mean 3.17
Std Dev 0.8618
h_dedx_estim2
Entries 59405
Mean 3.17
Std Dev 0.8614
h_dedx_estim2
Entries 59334
Mean 3.169
Std Dev 0.8603
Ratio
dE/dx, trunc40
DQM_V0001_R000000001__Global__mkFitOriginal__RECO
DQM_V0001_R000000001__Global__mkFitNewDett__RECO
DQM_V0001_R000000001__Global__mkFitNewDett33__RECO
DQM_V0001_R000000001__Global__mkFitNewDett04__RECO
Entries 59370
Mean 9.489
Std Dev 4.3
h_dedx_nom1
Entries 59438
Mean 9.487
Std Dev 4.299
h_dedx_nom1
Entries 59405
Mean 9.487
Std Dev 4.3
h_dedx_nom1
Entries 59334
Mean 9.489
Std Dev 4.3
Ratio
dE/dx number of measurements
_sat1
Entries 59370
Mean 0.8053
Std Dev 1.034
h_dedx_sat1
Entries 59438
Mean 0.8051
Std Dev 1.034
h_dedx_sat1
Entries 59405
Mean 0.8051
Std Dev 1.034
h_dedx_sat1
Entries 59334
Mean 0.8052
Std Dev 1.034
Ratio
dE/dx number of measurements with saturation