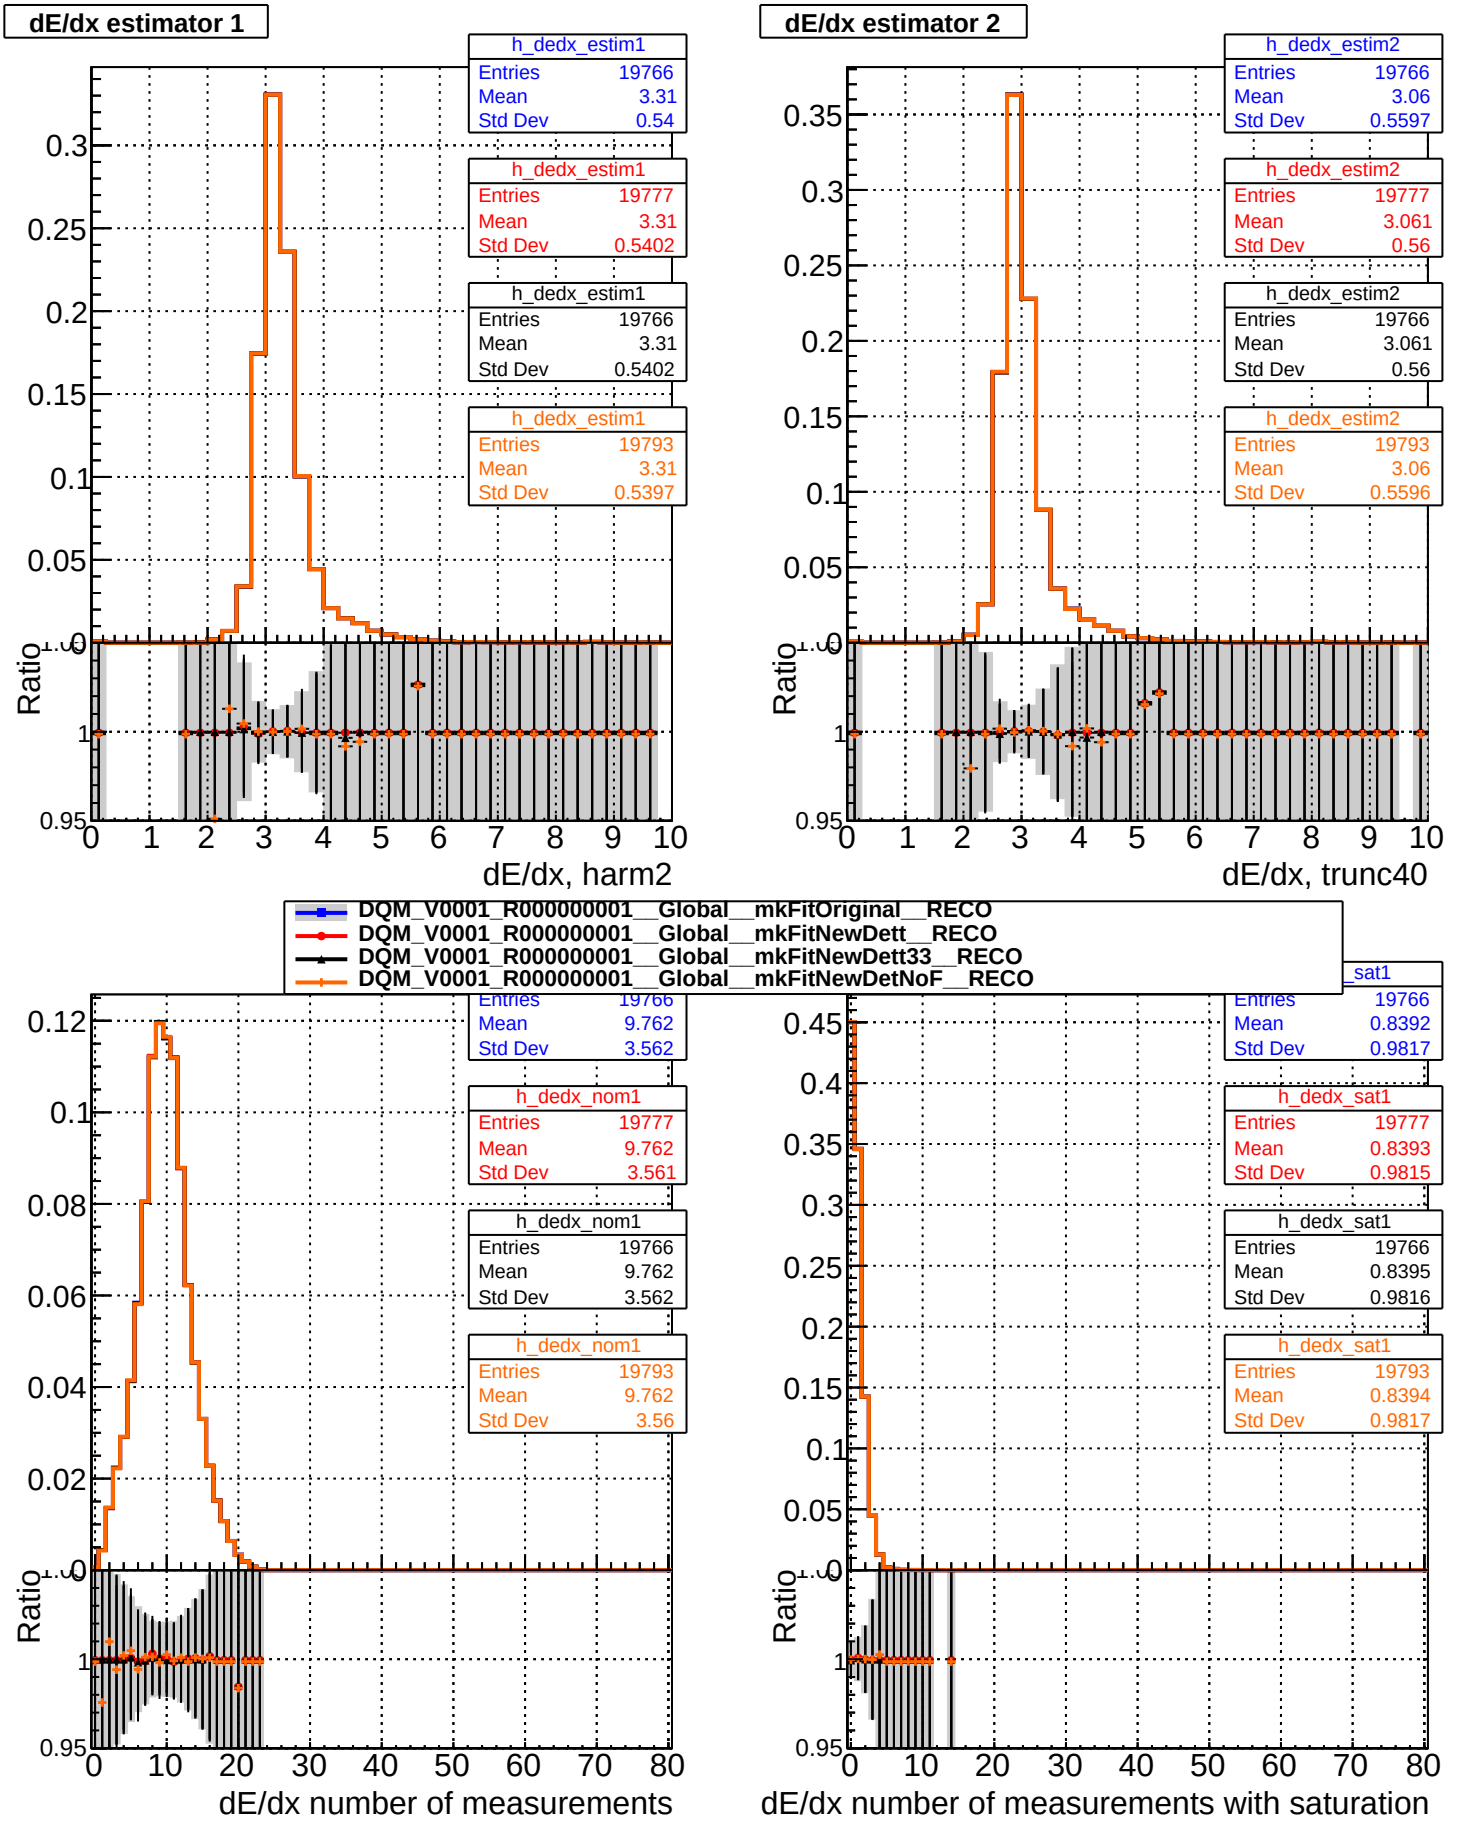
dE/dx estimator 1
h_dedx_estim1
Entries 19766
Mean 3.31
Std Dev 0.54
h_dedx_estim1
Entries 19777
Mean 3.31
Std Dev 0.5402
h_dedx_estim1
Entries 19766
Mean 3.31
Std Dev 0.5402
h_dedx_estim1
Entries 19793
Mean 3.31
Std Dev 0.5397
Ratio
dE/dx, harm2
dE/dx estimator 2
h_dedx_estim2
Entries 19766
Mean 3.06
Std Dev 0.5597
h_dedx_estim2
Entries 19777
Mean 3.061
Std Dev 0.56
h_dedx_estim2
Entries 19766
Mean 3.061
Std Dev 0.56
h_dedx_estim2
Entries 19793
Mean 3.06
Std Dev 0.5596
Ratio
dE/dx, trunc40
DQM_V0001_R000000001__Global__mkFitOriginal__RECO
DQM_V0001_R000000001__Global__mkFitNewDett__RECO
DQM_V0001_R000000001__Global__mkFitNewDett33__RECO
DQM_V0001_R000000001__Global__mkFitNewDetNoF__RECO
Entries 19766
Mean 9.762
Std Dev 3.562
h_dedx_nom1
Entries 19777
Mean 9.762
Std Dev 3.561
h_dedx_nom1
Entries 19766
Mean 9.762
Std Dev 3.562
h_dedx_nom1
Entries 19793
Mean 9.762
Std Dev 3.56
Ratio
dE/dx number of measurements
_sat1
Entries 19766
Mean 0.8392
Std Dev 0.9817
h_dedx_sat1
Entries 19777
Mean 0.8393
Std Dev 0.9815
h_dedx_sat1
Entries 19766
Mean 0.8395
Std Dev 0.9816
h_dedx_sat1
Entries 19793
Mean 0.8394
Std Dev 0.9817
Ratio
dE/dx number of measurements with saturation